Kontaktloses Digitales

INFRAROT THERMOMETER

VON

LyfTrack™

LyfTrack™

MODELL IR988

LCD-Display

Infrarot-Detektor

„Runter"-Taste

„Hoch"-Taste

„Set" Einstellungstaste

Schalter

Batterieabdeckung

150 mm

Modus

Gemessener Wert

Speicher

Signalton

Einheit

Letzte Daten
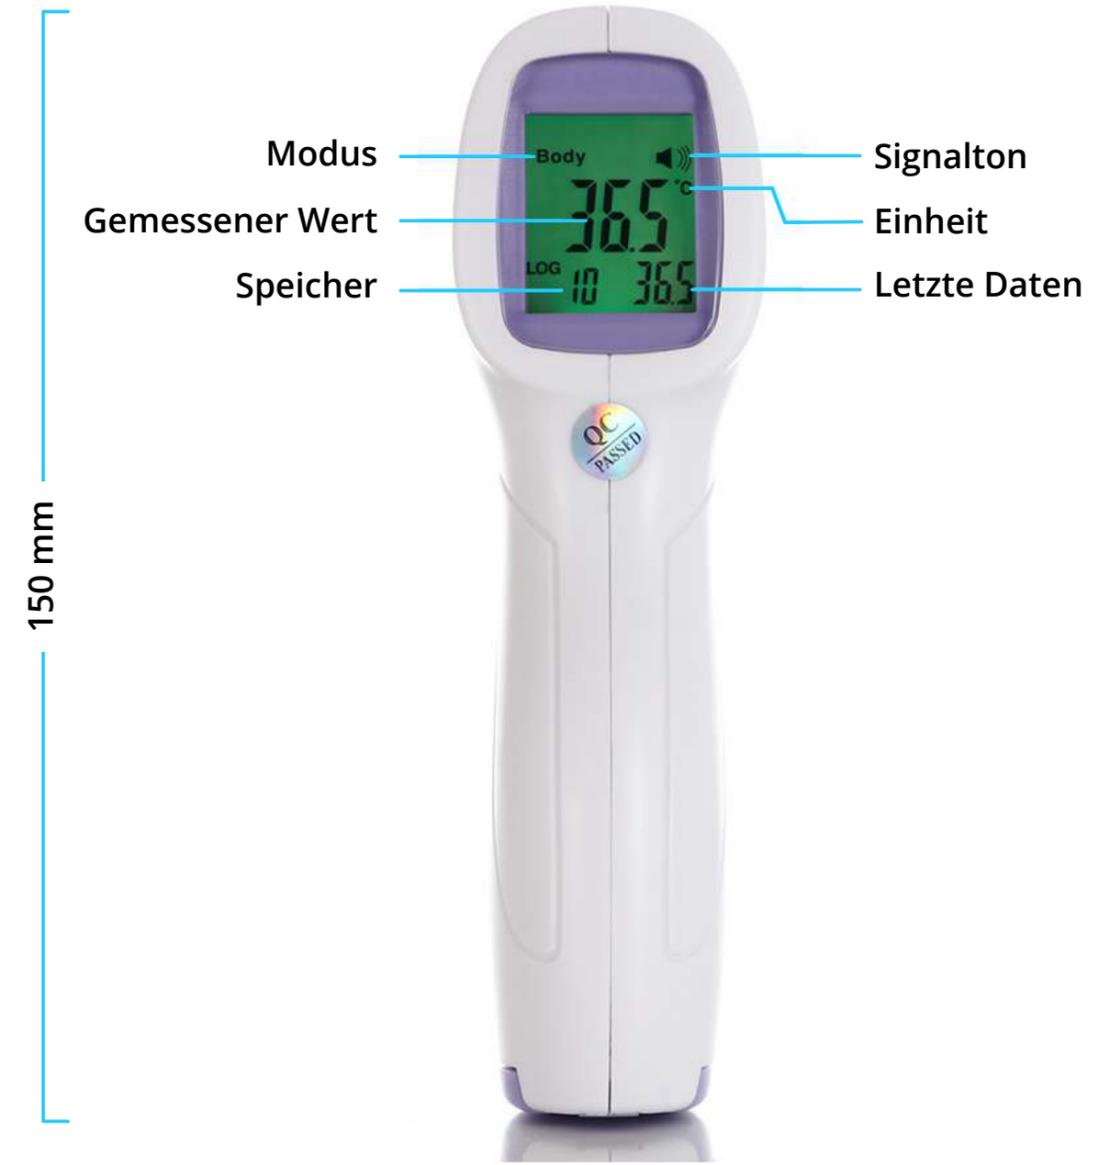
# PRODUKTEIGENSCHAFTEN

## MODELL IR988

1s
In 1 Sekunde

Smart-Chip

Intelligenter Sensor

32-Einheiten Speicherarray

Alarm bei hoher Temperatur

Infrarot Kontaktlos

Großbildschirm -Anzeige

3-Farben LED-Alarm mit Hintergrundbeleuchtung

Fieber-Signalton

°F / °C Modus
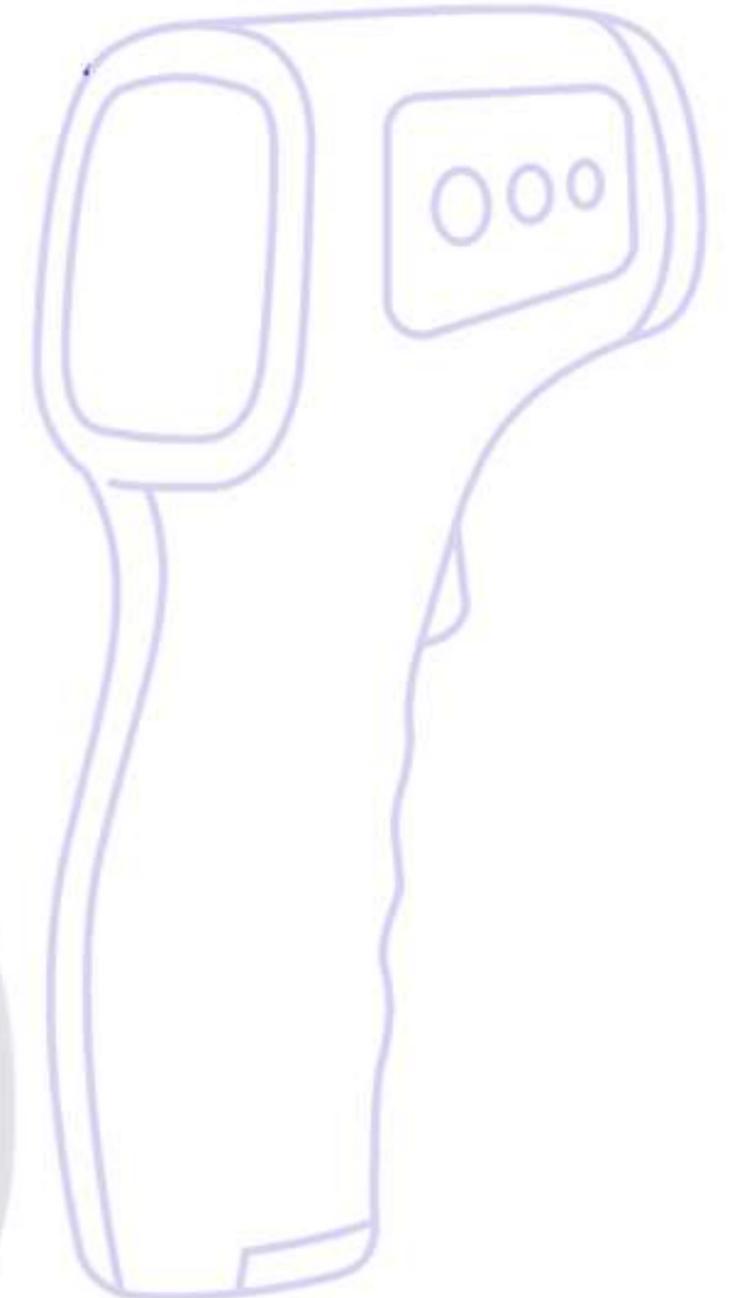
BESONDERE EIGENSCHAFTEN

3-Farben-LED-Alarm mit Hintergrundbeleuchtung

Im Menschenkörper-Modus kann das Produkt auf intelligente Weise die Messergebnisse anzeigen und mit verschiedenen im Hintergrund beleuchteten LED-Farben anfordern.

$32.0\,^{\circ}C \sim 37.4\,^{\circ}C$ (Grün)

$37.5\,^{\circ}C \sim 37.9\,^{\circ}C$ (Orange)

$38.0\,^{\circ}C \sim 42.9\,^{\circ}C$ (Rot)

Signalton für hohes Fieber

Sobald die Temperatur 38°C / 100.4°F übersteigt, wird ein Ton ausgegeben der signalisieren soll, dass die Temperatur nicht normal ist.

PRODUKTVERWENDUNG

Menschenmenge

Supermarkt

Öffentliche Orte

Unternehmen & Institutionen

Babys

Familie

Objekte

Haustiere

PRODUKTZERTIFIKATE

LyfTrack™

Attestation of Conformity

No. ICR Polska/////////

CE

Name and address of Registered Manufacturer: ////////

Product name: Non-contact infrared thermometer

Product type/model: IR988

Trade mark: N.A.

This Attestation confirms that the product meets the requirements of the following normative documents and within limits of its documents gives presumption of conformity with essential requirements of Directive 93/42/EEC.

Relevant EC Directive: Medical Device Directive 93/42/EEC

Conformity assessment procedure: EC Declaration of Conformity (Annex VII of Directive 93/42/EEC)

Classification: Class I according Rule 1 of Annex IX of Directive 93/42/EEC

Applied normative documents: EN 60601-1: 2006 / EN 60601-1-2: 2015

Applied Quality Management System n/a

This AoC will remain valid only if Quality Management System Certificate remains valid. The assessment process has been carried out in accordance with the program PC-P-07-07. Evaluation has been carried out in accordance with test report made by:
• CHINA CERREI (SICHUAN) LABORATORY

No. of test report: SC(20)-50165A-10-2-MDD

Issue date: 25.03.2020

Expiration date: 24.03.2025

The mutual obligations and rights of the certification are regulated by the contract No. ICR Polska/2020-3125.

This Attestation applies to products having the same attributes (parameters), intended use, that have been evaluated and meet the requirements of the aforementioned standard.

Director: Rafał Kalinowski

Warsaw, 25. 03. 2020.

ICR Polska Co. Ltd.
ul. Plac Przymierza 6, 03-944 Warszawa
www.icrpolska.com, e-mail: icrpolska@icrqa.com

CERTIFICATE OF EMC COMPLIANCE

According to Directive: 2014/30/EU

Ref. No.: ////////

Applicant: ////////
Address: ////////

Manufacturer: ////////
Address: ////////

Product: Non-contact infrared thermometer

Brand Name: ////

Model No.: IR988

The test sample of product has been passed, the test according to requirements of the following standards:

Standard(s):
EN 60601-1-2:2007
EN 61000-3-2 :2006+A1:2009+A2:2009
EN 61000-3-3 :2013

Test report(s) No.: ////////

Based on the voluntary assessment of the product sample and technical file, we confirm that the above-mentioned product meets the requirements of the EC directive.
The CE mark as show below can be used, under the responsibility of the manufacturer or the importer, after completion of an EC declaration of conformity and compliance with all relevant EC directives.

CE

Approved by/Date: Mar. 11, 2020

Shenzhen iTC Product Testing Co., Ltd.
2nd Floor, Building A7, Xinhe XinxingThird Industrial Area, Fuhai Road, Fuyong Street Bao'an District, Shenzhen, China
Tel: (86)-0755-33138690 Fax: (86)-0755-23071003 http://www.itclab.cn/

FCC TEST REPORT

Shenzhen iTC Product Testing Co., Ltd.

Report No.: ////////

Client Information:

Applicant: ////////
Applicant add.: ////////
Brand Name: ////

Product Information:

Product Name: Non-contact infrared thermometer

Model No.: IR988

Derivative model No.: N/A

Test Date: Mar. 06, 2020 to Mar. 13, 2020 **Issue Date:** Mar. 13, 2020

Test Standard: FCC Part 15, Subpart B: 2016 / ANSI C63.4:2014

Test Result: PASS

Tested by Amanda Chen — Amanda Chen

Reviewed by Apple Huang — Apple Huang

Approved by John Liu — John Liu

This test report may be reproduced in full only
Test result presented in this test report is applicable to the tested sample only

PRODUKTZERTIFIKATE

Certificate 1 — FDA Certification of Registration

Fiscal Year 2020

CERTIFICATION OF REGISTRATION

This certifies that:

Model No: IR988

Was registered with US Food and Drug Administration, Center for Devices and Radiological Health, pursuit to the Code of Federal Regulations 21 CFR 807, by Shenzhen Huacetong Testing and Certification Co., ltd

Owner/Operator Number:
Device Listing#: See annex
Expiration Date: December. 31, 2020

Shenzhen Huacetong Testing and Certification Co., ltd. will confirm that such registration remains effective upon request and presentation of this certificate

until the end of the calendar year stated above, unless said registration is terminated after issuance of this

certificate. Shenzhen Huacetong Testing and Certification Co., ltd makes no other representations or warranties,

nor does this certificate make any

representations or warranties to any person or entity other than the named certificate holder, for whose sole

benefit it is issued. This certificate does not denote endorsement or approval of the certificate-holder's device or

establishment by the U.S. Food and Drug Administration. Shenzhen Huacetong Testing and Certification Co., ltd

assumes no liability to any person or entity in

connection with the foregoing.

Pursuant to 21 CFR 807.39, "Registration of a device establishment or assignment of a registration number

does not in any way denote approval of the establishment or its products. Any representation that creates an

impression of official approval because of registration or possession of a registration number is misleading and

constitutes misbranding." The U.S. Food and Drug Administration does not issue a certificate of registration,

nor does the U.S. Food and Drug Administration recognize a certificate of registration, Shenzhen Huacetong

Testing and Certification Co., ltd is not affiliated with the U.S. Food and Drug Administration.

Executive Director
Issued: Mar.30, 2020
Expiration Date: Dec.31, 2020

FDA

Certificate 2 — iTC Certificate of Compliance

CERTIFICATE OF COMPLIANCE

2015/863/EU Restriction of Hazardous Substance
Ref. No.:

Applicant:
Address:

Manufacturer:
Address:

Product : Non-contact infrared thermometer

Brand Name:

Model No.: IR988

The test sample of product has been passed, the test according to requirements of the following standards:

Standard(s):   Test report(s) No.:
IEC62321-3-1:2013;
IEC62321-4:2013+A1:2017;
IEC 62321-5:2013; IEC 62321-6:2015;
IEC 62321-7-1:2015;IEC 62321-7-2:2017;
IEC 62321-8:2017

The Certificate of compliance is based on a test procedure or an evaluation of the above-mentioned product. This is to certify that the above-mentioned product is in compliance with the EU RoHS Directive 2011/65/EU and its amendment directives 2015/863/EU (RoHS 2.0) of the European parliament.

ROHS

Approved by/Date: Mar. 13, 2020
Department Manager

Shenzhen iTC Product Testing Co., Ltd.
2nd Floor, Building A7 , Xinhe XinxingThird Industrial Area, Fuhai Road, Fuyong Street Bao'an District, Shenzhen, China
Tel: (86)-0755-33138690   Fax: (86)-0755-23071003   http://www.itclab.cn/

Certificate 3 — Certificate of Accreditation

CERTIFICATE OF ACCREDITATION

ISP CERTIFICATION / UKAS

Medical device quality management system

Registration No.

We hereby certify that

ISO 13485:2016

Scope of certification/registration

Medical Devices, non-contact infrared temperature detector, electronic products, health measurement device research and development, production and sales

Issue date of this certificate:Mar 17, 2020 Valid date of this certificate:Mar 16, 2021

First registration:Mar 17, 2020 Registration deadline: Mar 16, 2023

(The effectiveness of this certificate shall be validated by periodic surveillance audit of ISP for maintenance.

The intervals of not more than 12 months, Conditions on effectiveness of certificate see http://www.isp-acpc.com

Note: the use of outside mainland China)

IAF   **UKAS**   Issued by:

INSPEC INTERNATIONAL
www.isp-acpc.com

PRODUKTVERPACKUNG

Für Menschen	Unbegrenzte Menschenmenge	Speicher-Array	32 Einheiten
Messverfahren	Kontaktlos	Stromversorgung	DC3V (AAA*2)
Messstelle	Stirn	Größe	150*81*41mm
Messabstand	3~5cm	Gewicht	105.5g
Messbereich	Körper: 34.8°C~42.5°C Objekte: 0°C~93°C (±1°C)	Max. zulässiger Fehler	35°C~42.0°C (±0.2°C) Others (±0.3°C)

Informationen zum Paket	Menge: 50Stücke/Karton	Kartongröße: 58*27*39.5cm
	Bruttogewicht: 8.2KG/Carton	Kartonvolumen: 0.06186CBM

Schranktyp	20' GP	40' GP	40' HC/HQ
Kartonmenge	533	1075	1233
Produktmenge	26650	53750	61650
Volumen (tatsächliche Passform)	32.97138	66.4995	76.27338

Batterien sind nicht im Paket enthalten